



Liquid Turbine Flow Meter

User Manual





Content

1.0 GENERAL INFORMATION	1
2.0 SPECIFICATIONS	
3.0 OPERATION CONDITIONS	3
4.0 CAUTIONS FOR INSTALLATION	5
5.0 DIMENSION	8
6.0 ELECTRICAL WIRING	.11
7.0 OPERATION AND SETUP	16
8.0 TROUBLESHOOTING	.19
9.0 METER CONSTRUCTION	. 20



Warning

When the flow meter is installed at explosion hazard field, DON'T remove the COVERPLATE when the meter is powered. Please make parameter setting at safe filed prior to installation.



Special Notices

Pictures & Descriptions are for your information only, please refer to the actual product. Parameters are subjected to changes without notice.



1.0 GENERAL INFORMATION

This manual will assist you in installing, using and maintaining your turbine flow meter. It is your responsibility to make that all operators have access to adequate instructions about safe operating and maintenance procedure.



Warning

For your safety, review the major warnings and cautions below before operating your equipment

Use only fluids that are compatible with the housing material and wetted components of your turbine.

During turbine removal, liquid may spill. Follow the liquid manufacturer's safety precautions for clean up of minor spills.

When measuring flammable liquids, observe precautions against fire or explosion.

Do not blow compressed air through the turbine.

When handling hazardous liquids, always follow the liquid manufacturer's safety precautions.

Handle the rotor carefully. Even small scratches or nicks can affect accuracy.

When working in hazardous environments, always exercise appropriate safety precautions.

When tightening the turbine, use a wrench only on the wrench flats .

For best results, calibrate the meter at least 1 time per year.

Product Description

HLY series turbine flow meters have the features: high accuracy, good repeatability, convenient installation/maintenance, simple structure etc.

Liquid flows through the turbine housing causing an internal rotor to spin. As the rotor spins, an electrical signal is generated in the pickup coil. This signal is converted into engineering units (liters, cubic meters, gallons etc.) on the local display where is applicable. Optional accessory modules can be used to export the signal to other equipment.

Upon receipt, examine your meter for visible damage. The turbine is a precision measuring instrument and should be handled carefully. Remove the protective plugs and caps for a thorough inspection. If any items are damaged or missing, contact

Make the turbine flow model meets your specific needs. For your future reference, it might be useful to record this information on nameplate in the manual in case it becomes unreadable on the turbine. Refer to the nameplate for your customized product's specification.

1



2.0 SPECIFICATIONS

Performance

Repeatability: ±0.2%

Accuracy: Standard: ±1% of reading;

Optional: ±0.5% of reading

Wetted Components

Housing: Standard - 304 Stainless Steel

Optional - 316 Stainless Steel

Bearings and Shaft: Tungsten Carbide

Rotor: Standard - 2Cr13 Stainless Steel

(Optional Alloy CD4Mcu)

Retaining Rings: 316 Stainless Steel

Output Signal: (Where applicable)

Sensor: Pulse signal (Low Level: ≤0.8V; High Level: ≥8V)

Transmitter: 4 to 20 mA DC current signal

Signal Transmission Distance: ≤1,000 m

Electrical Connections:

Basic Type: Hirschmann Connector or three-core cable

Explosion Proof Type: ISO M20×1.5 Female

Explosion Proof Level:

Standard: None

Optional: ExdIICT6

Protection Level: IP65



3.0 OPERATION CONDITIONS

Ambient:

Temperature: -10°C to +55°C

Pressure: 86 to 106 KPa

Relative Humidity: 5% to 90%

Power Supply:

Sensor: +12V DC (Optional: +24V DC)

Transmitter: +24V DC

Field Display Type B: Integral 3.2V Lithium Battery (Others available on request)

Field Display Type C: +24V DC

Fluid Temperature and Pres:

Temperature: -20°C to +110°C

Pres: Fluid pres should be limited according to rating.

Measurable Flow Rate Range and Pres Level: (See table 1)

Table 1. Measurable Flow Rage Range and Pressure Rating

Nominal Standard Flow Range (SFR)		Extended Flow Range (EFR)	Standard Pres Rating	Customized Pres Rating	
(mm)	(in.)	(m³/h)	(m³/h)	(MPa)	(MPa) - Flange Fitting
4	0.15	0.04 to 0.25	0.04 to 0.4	Thread: 6.3	12, 16, 25
6	0.25	0.1 to 0.6	0.06 to 0.6	Thread: 6.3	12, 16, 25
10	0.4	0.2 to 1.2	0.15 to 1.5	Thread: 6.3	12, 16, 25
15	0.5	0.6 to 6	0.4 to 8	Thread: 6.3; Flange: 2.5	4.0, 6.3, 12, 16, 25
20	0.75	0.8 to 8	0.45 to 9	Thread: 6.3; Flange: 2.5	4.0, 6.3, 12, 16, 25
25	1	1 to 10	0.5 to 10	Thread: 6.3; Flange: 2.5	4.0, 6.3, 12, 16, 25
32	1.25	1.5 to 15	0.8 to 15	Thread: 6.3; Flange: 2.5	4.0, 6.3, 12, 16, 25
40	1.5	2 to 20	1 to 30	Thread: 6.3; Flange: 2.5	4.0, 6.3, 12, 16, 25
50	2	4 to 40	2 to 40	Flange: 2.5	4.0, 6.3, 12, 16, 25
65	2.5	7 to 70	4 to 70	Flange: 2.5	4.0, 6.3, 12, 16, 25
80	3	10 to 100	5 to 100	Flange: 2.5	4.0, 6.3, 12, 16, 25
100	4	20 to 200	10 to 200	Flange: 1.6	4.0, 6.3, 12, 16, 25
125	5	25 to 250	13 to 250	Flange: 1.6	2.5, 4.0, 6.3, 12, 16
150	6	30 to 300	15 to 300	Flange: 1.6	2.5, 4.0, 6.3, 12, 16
200	8	80 to 800	40 to 800	Flange: 1.6	2.5, 4.0, 6.3, 12, 16



Model Selection

HIV-	Model No.								Definition.		
Section Sect	HLY-		/□	/□	/□	/□	/□	/□	/□	/□	Definition
10		4									DN4
15		6									DN6
Nominal 32		10									DN10
Nominal		15									DN15
Nominal diameter (mm)		20									DN20
DN40 DN50		25									DN25
(mm) 50 BNSO 80 100 DNSO 100 DN100 DN125 DN200 DN200 DN200 Meter type FL LW JZ A A G1 Threaded Clamp-on by flange 24V power supply, no field display, pulse output 24V power supply, no field display, no output Battery powered, field display, no output External power supply, field display, no output (Explosion-proof type) Battery powered, field display, no output (Explosion-proof type) External power supply, field display, no output (Explosion-proof type) External power supply, field display, no output (Explosion-proof type) External power supply, field display, no output (Explosion-proof type) External power supply, field display, no output (Explosion-proof type) External power supply, field display, no output (Explosion-proof type) External power supply, field display, no output (Explosion-proof type) External power supply, field display, no output (Explosion-proof type) External power supply, field display, no output (Explosion-proof type) External power supply, field display, no output (Explosion-proof type) External power supply, field display, no output (Explosion-proof type) External power supply, field display, no output (Explosion-proof type) External power supply, field display, no output (Explosion-proof type) External power supply, field display, no output (Explosion-proof type) External power supply, field display, no output (Explosion-proof type) External power supply, field display, no output (Explosion-proof type) External power supply, field display, no output (Explosion-proof type) External power supply, field display, no output (Explosion-proof type) External power supply, field display, no output (Explosion-proof type) External power	Nominal	32									DN32
DN65 DN80 DN100 DN125 DN150 DN200 Flanged DN100 DN200 Flanged DN100 DN200 Flanged DN100 DN200 Flanged DN100 DN200	diameter	40									DN40
Note the content of	(mm)	50									DN50
100		65									DN65
125 150 200		80									DN80
150		100									DN100
DN200 Flanged Threaded Clamp-on by flange 24V power supply, no field display, pulse output 24V power supply, field display, A-20mA output Battery powered, field display, no output External power supply, field display, no output (Explosion-proof type)Battery powered, field display, no output (Explosion-proof type)Batt		125									DN125
FL Connection FL LW JZ		150									DN150
Connection LW JZ N A A G1 G1 GX A GX E1 BThreaded Clamp-on by flange 24V power supply, no field display, pulse output 24V power supply, field display, 4-20mA output Battery powered, field display, no output External power supply, field display, no output (Explosion-proof type)Battery powered, field display, no output (Explosion-proof type)Battery powered, field display, no output (Explosion-proof type)Battery powered, field display, no output (Explosion-proof type) External power supply, field display, RS485/current/pulse output Standard range Extended range Special range 0.5 1.0 0.2(by customized, long production period) 304 SS 316(L) SS 2Cr13 impeller Duplex steel impeller Non-explosion proof Exd II CT6 Gb N Standard		200									DN200
Meter type S			FL								Flanged
Meter type N	Connection		LW								Threaded
Meter type A G1			JZ								Clamp-on by flange
Meter type G1				N							24V power supply, no field display, pulse output
Meter type G1				Α							24V power supply, field display, 4-20mA output
Meter type Columbia				G1							
Meter type Columbia											External power supply field display.
E1 EX EX EX EX EX EX EX EX	Meter type			GX							
display, no output (Explosion-proof type) External power supply, field display, RS485/current/pulse output Standard range Extended range Extended range Special range 0.5 1.0 0.2(by customized, long production period) 304 SS 316(L) SS 2Cr13 impeller Duplex steel impeller Duplex steel impeller Explosion-proof grade Temperature and pressure resistant Explosion Figure Figur											·
Accuracy D5 Accuracy 10 D2 Range Meter material Impeller material Explosion-proof grade S				E1							
Accuracy D5 Accuracy 10 D2 Range Meter material Impeller material Explosion-proof grade S				5 1/							(Explosion-proof type) External power
Accuracy 10 02 Range Special range 0.5 1.0 0.2(by customized, long production period) 304 SS 316(L) SS 2Cr13 impeller Duplex steel impeller Duplex steel impeller Non-explosion proof Exd II CT6 Gb N Standard				EX							
Range Special range 0.5 1.0 0.2(by customized, long production period) 304 SS 316(L) SS 2Cr13 impeller Duplex steel impeller Duplex steel impeller Non-explosion proof Explosion-proof grade Temperature and pressure resistant S L N Standard					05	1					Standard range
Range S W Z Meter material S L S L S L S L S L S L S L S	Accuracy				10						Extended range
Range M Z					02						Special range
Temperature and pressure resistant Description: Z						S					0.5
Description of the second of	Range					W					1.0
Meter material Impeller material S Impeller material Explosion-proof grade S Impeller material Impeller material S Impeller material Impell						Z					0.2(by customized, long production period)
Meter material Impeller material S Impeller material Explosion-proof grade Impeller material Impeller m							S				304 SS
Impeller material S L Duplex steel impeller Duplex steel impeller Non-explosion proof Exd II CT6 Gb N Standard	Meter mate	erial					L				
Duplex steel impeller							_	S			• •
Explosion-proof grade N	Impeller ma	│ Imneller material ├──									
Explosion-proof grade E Exd II CT6 Gb N Standard									N		
Temperature and pressure resistant N Standard	Explosion-p	roof gr	ade								·
Temperature and pressure resistant										N	
HIVI HIGH NYESSIIYA	Temperatu	re and	pressu	re resi	stant					H(_x)	High pressure

Notes: DN20,DN32,DN65,DN125 are custom. X refers to number(s), standing for different functions. Contact us for details.



4.0 CAUTIONS FOR INSTALLATION

Mounting Positions

Turbine flow meters should be installed at the place in compliance with the requirements below:

- ♦ Easy maintenance
- ♦ No vibration

- ♦ No electromagnetic interface
- Away from heat source

Mounting Orientation

All turbine flow meters are designed to measure flow in only one direction. The direction is indicated by the arrow on the body.

Required Lengths of Straight Runs

Flow altering device such as elbows, valves and reducers can affect accuracy. See diagram 1 for typical flow meter system installation.

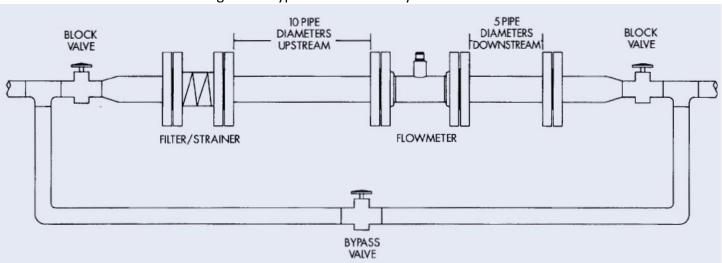


Diagram 1. Typical Flow Meter System Installation


The recommended guidelines are given to enhance accuracy and maximize performance. Distance given here are minimum requirements; double them for desired straight pipe lengths.

- Upstream: allow a minimum straight pipe length at least 10 times the internal diameter of the pipe. For example, with the 50mm pipe, there should be 500mm of straight pipe immediately upstream.
 Desired upstream straight pipe length is 1000mm.
- Downstream: allow a minimum straight pipe length at least 5 times the internal diameter of the pipe.
 For example, with the 50mm pipe, there should be 250mm of straight pipe immediately upstream.
 Desired upstream straight pipe length is 500mm



See diagram 2 for straight pipe length requirement when there is altering device.

Diagram 2. Number of Pipe Diameter (D=Diameter)

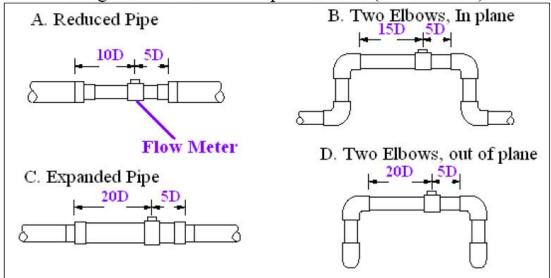



Warning: Precaution for direct sunshine and rain when the meter is installed outside.

Anti-Cavitation

Cavitation can be caused by entrained air, and it can seriously damage the rotor on a turbine flow meter. An amount higher than about 100 mg/l of entrained air or gas can produce error. In addition, cavitations can be caused by too little back pres on the flow meter. For turbine flow meters, you should provide a back pres (downstream pres) of at least 1.25 times the vapor pres, plus 2 times the pressure drop through the flow meter. See formula 1.

Formula 1:
$$P_b \ge 1.25 \times P_v + 2 \times (P_{in} - P_{out})$$

In formula 1: $(P_b: Back pres; P_v: Vapor Pres; P_{in}: Inlet Pres; P_{out}: Outlet Pres)$

Create back pres by installing a control valve on the downstream side of the meter at the proper distance detailed above.



Special Notice

- Foreign material in the liquid being mead can clog the meter's rotor and adversely affect accuracy. If this problem is anticipated or experienced, install screens to filter impurities from incoming liquids.
- ♦ To en accurate measurement, drain all air from the system before use.
- When the meter contain removable cover plates. Leave the cover plate installed unless accessory modules specify removal. Don't remove the cover plates when the meter is powered, or electrical shock and explosion hazard can be caused.



Thread Connections

- 1. To protect against leakage, seal all threads with an appropriate sealing compound. Make the sealing compound does not intrude into the flow path.
- 2. Make the arrow on the outlet is pointed in the direction of the flow.
- 3. Tighten the turbine onto the fittings. Use a wrench only on wrench flats.

Flange Connections

For standard product, the flange follows GB/T 9119-2000 (ISO 7005-1) RF (Raised Face).

Note: flange can be customized following other criteria.


Use a gasket between the meter flange and mating flange. Determine the material of the gasket based on the operating conditions and type of fluid.

Note: Do not over tighten the flange bolts. This may cause the gasket to be compressed into the flow stream and may decrease the accuracy of the meter.



5. INSTALLATION DIMENSIONS

Thread or flange connection is used according to different flow models.

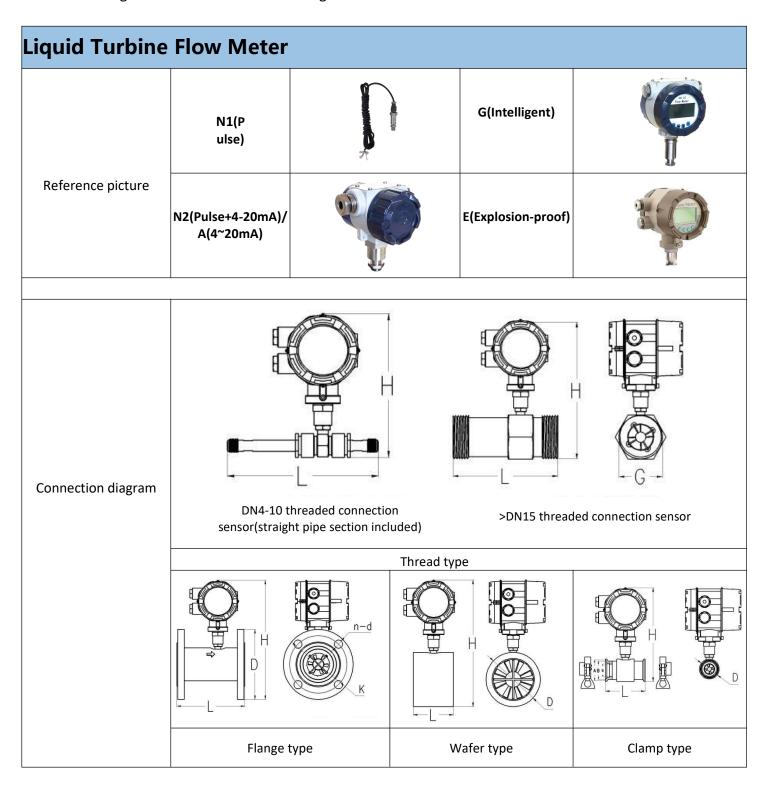



Threaded and flanged type of liquid turbine flow meter

Threaded connection

	L		G			
DN(mm)	DN(mm) (mm)		N2(Pulse+4-20mA)/ A(4~20mA)	G(Intelligent)	E(Explosion-proof)	
4	225	145	145	190	210	G1/2
6	225	145	145	190	210	G1/2
10	345	150	150	190	210	G1/2
15	75	150	150	195	215	G1
20	85	155	155	200	220	G1
25	100	160	160	205	225	G11/4
32	140	180	180	225	245	G2
40	140	185	185	230	250	G2
50	150	190	190	235	255	G21/2

Note: for DN4~DN10, when connecting the filter, the overall length should be increased by 50mm on the basis of L..

Flanged Connection

DN	L	D	К		р	n			
(mm)	(mm)	(mm)	(mm)	N1 (Pulse)	N2(Pulse+4-20mA)/ A(4~20mA)	G(Intelligent)	E(Explosion- proof)	(mm)	(Qty of holes)
15	75	95	65	175	180	225	245	14	4
20	80	105	75	185	190	235	255	14	4
25	100	115	85	200	195	240	260	14	4
32	140	140	100	210	215	260	280	18	4
40	140	150	110	195	220	265	285	18	4
50	150	165	125	230	235	280	300	18	4
65	170	185	145	255	260	305	325	18	4
80	200	200	160	260	265	310	330	18	8
100	220	220	180	285	285	330	350	18	8
125	250	250	210	310	315	360	380	18	8
150	300	285	240	345	345	390	410	22	8
200	350	340	295	395	400	445	465	22	12



Wafer and clamp types of liquid turbine flow meter

	L		D					H(mm)			
DN(mm))		(mm)	N2(P	ulse+4-20	mA)	A(4~20m		igent)	E(Explo	sion-proof)
4	50	0	38					26!			215
6	50	0	38					26	5		215
10	50	0	38					26!	5		215
15	5.	5	47					27!	5		225
20	6	0	53					280)		230
25	6	0	58					28!	5		235
32	7(0	66			Χ		290)		240
40	7(0	72					300)		250
50	7(0	92					31!	5		265
65	80	0	100		210		210	25!	5		275
80	9(0	112		225		225	270)		290
100	10	00	137		250		250	29!	5		315
125	12	20	165		275		275	320)		340
150	15	0	190		300		300	34!	5		365
200	15	0	243		350		350	39!	5		415
DN(mm)	L(mm)	D(mm)	A(mm)	B(mm)	B(mm)	N2(Pu	ulse+4-20			lligent)	E(Explosion
							,				-proof)
											215
	50										215
											215
											225
	100	50.5	46	40.5							225
											230
				F0 -							230
									1		245
50	150	78	73.5	68	50		190	190		35	255
65	170	91	86	80.5	65		205	205		50	270
		106	100.5	94 106	80 100		220 240	220		65 85	285 305
80	200	127	113					2711			
	6 10 15 20 25 32 40 50 65 80 100 125 150 200	6 50 10 50 15 55 20 60 25 60 32 70 40 70 50 70 65 80 80 90 100 100 125 12 150 15 200 15 DN(mm) L(mm) 4 6 50 10 15 20 100 25 32 120	6 50 10 50 15 55 20 60 25 60 32 70 40 70 50 70 65 80 80 90 100 100 125 120 150 150 200 150 DN(mm) L(mm) D(mm) 4 6 50 10 15 20 100 50.5 32 120	6 50 38 10 50 38 15 55 47 20 60 53 25 60 58 32 70 66 40 70 72 50 70 92 65 80 100 80 90 112 100 100 137 125 120 165 150 150 190 200 150 243 DN(mm) L(mm) D(mm) A(mm) 4 6 50 10 15 20 100 50.5 46 25 32 120	6 50 38 10 50 38 15 55 47 20 60 53 25 60 58 32 70 66 40 70 72 50 70 92 65 80 100 80 90 112 100 100 137 125 120 165 150 150 190 200 150 243 DN(mm) L(mm) D(mm) A(mm) B(mm) 4 6 50 10 15 20 20 100 50.5 46 40.5 32 120	6 50 38 10 50 38 15 55 47 20 60 53 25 60 58 32 70 66 40 70 72 50 70 92 65 80 100 210 80 90 112 225 100 100 137 250 125 120 165 275 150 150 190 300 200 150 243 350 DN(mm) L(mm) D(mm) A(mm) B(mm) B(mm) 4 6 10 15 20 100 50.5 46 40.5 20 25 32 120 32	6 50 38 10 50 38 15 55 47 20 60 53 25 60 58 32 70 66 40 70 72 50 70 92 65 80 100 210 80 90 112 225 100 100 137 250 125 120 165 275 150 150 190 300 200 150 243 350 A 6 6 10 15 15 15 15 15 15 15	6 50 38 10 50 38 15 55 47 20 60 53 25 60 58 32 70 66 X 40 70 72 50 70 92 65 80 100 210 210 80 90 112 225 225 100 100 137 250 250 125 120 165 275 275 150 150 190 300 300 200 150 243 350 350 DN(mm) L(mm) D(mm) A(mm) B(mm) B(mm) N2(Pulse+4-20 mA) 4 150 6 150 10 150 150 150 150 15 160 20 160 25 165 32 120 120 165 32 165	6 50 38 10 50 38 15 55 47 20 60 53 25 60 58 32 70 66 40 70 72 50 70 92 65 80 100 210 210 250 80 90 112 225 225 225 270 100 100 137 250 250 290 125 120 165 275 275 321 150 150 190 300 300 340 200 150 243 350 350 391	Column	Column



6.0 ELECTRICAL WIRING

Warning: Electrical Hazard

Disconnect power before beginning installation.


Turbine Flow Sensor/Transmitter


♦ 1. Pulse Type without Explosion Proof

Terminal wiring


Terminal Symbols	Description					
Red Wire	Power Supply: "24V+"					
White Wire	Power Supply: "24V-"					
Yellow Wire	Pulse Output					

♦ 2. Pulse with Explosion Proof:





- Notice: (1) High level amplitude >22V
 - (2) Low level amplitude<0.8V
 - (3) Load capacity>1100 Ω
 - (4) Pulse frequency≤3000Hz
- ♦ 3. 4-20mA Output with Explosion Proof Type

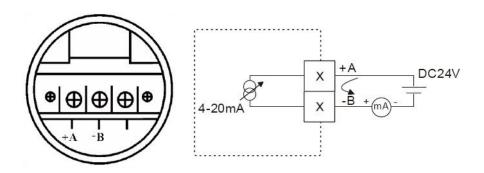

Notice: Load resistor is <




◆ 4. Function table for the Intelligent display type

		Output								
Main Power	Display	Pulse Scaled Pulse Pulse *1 *2		2-wire 4~20 mA	3-wire 4-20 mA	4-wire 0 -20m	4-wire 4~20m A	Modbus RS485		
Battery*3	•	•								
24V DC	•	•	•	•	0			•		
24V C+Battery*4	•	•	•	•	0			•		
220Vac	•	•	•			0	•	•		
Description of the	symbols:		Def	ault Functi	on	0	Optional			

Notice:

- 1. The pulse means the signal which is in direct proportion to the impeller speed.
- 2. The scaled Pulse means the signal when the flow rate reach ONE unit volume(m3, L, 0.01L...)
- 3. The batter model is ER34615
- 4. The battery model is ER26500

4.1 24V DC powered type

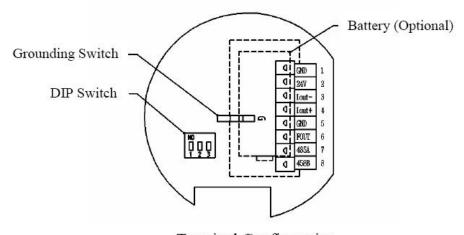


Terminal Configuration



Terminal Configuration

Terminal No.	Terminal Symbols	Description
1	GND	
2	24V	24V+ DC Power Supply
3	lout-	Current Output 4 to 20 mA DC (+) (2Wire)
4	lout+	
5	GND	24V- DC Power Supply
6	-FOUT	F-OUT: Pulse output
7	485A	RS485-
8	485B	RS485+


$4.1.1\,$ Pulse / Scaled Pulse output

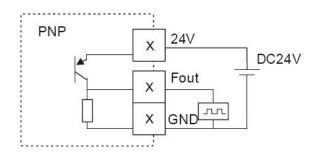

Notice: (1) High level amplitude >22V


- (2) Low level amplitude<0.8V
- (3) Load capacity>1100Ω
- (4) Pulse frequency≤3000Hz

4.1.2 (2 Wire) 4-20mA Output

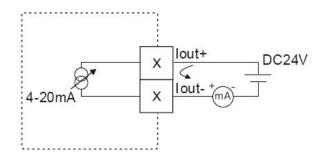




4.1.3 (3 Wire) 4-20mA Output

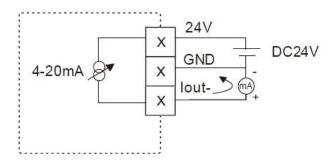


4.1.4 (3 Wire) 0-20mA Output

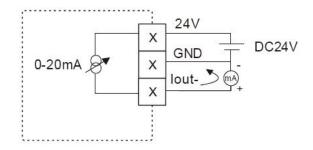


Notice: Load resistor is $<500\Omega$

4.1.5 RS485 communication

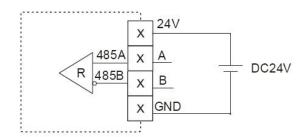

Notice: The communication format is Modbus-RTU protocol

4.2 220Vac powered type

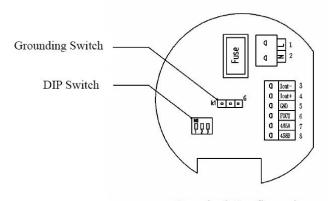


Terminal Configuration



Terminal	Configu	ration
	~~n	


Terminal No.	Terminal Symbols	Description
1	L	AC 220V Power Supply
2	N	AC 220V Power Supply
3	lout-	Current Output
4	lout+	Current Output
5	GND	Current / Pulse output -
6	FOUT	FOUT: Pulse output
7	485A	RS485-
8	485B	RS485+

4.2.1 Pulse / Scaled Pulse output

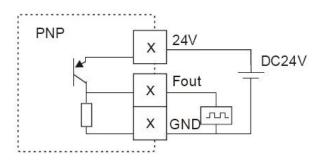


Notice: Three conditions are necessary for pulse output High level amplitude >22V Low level amplitude <0.8V Load capacity>1100 Ω Pulse frequency \leq 3000H

4.2.2 (4 Wire) 4-20mA Output

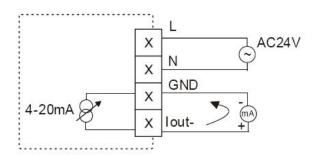


4.2.3 (4 Wire) 0-20mA Output

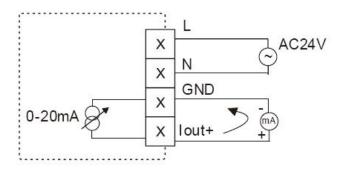




4.2.4 RS485 communication

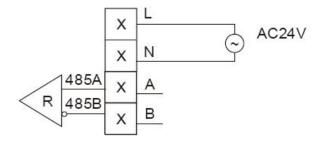

4.2.5 Function table for

DIP Switch: K1										
Function	1	2	3							
Original Pulse Output	ON	OFF	OFF							
Scaled Pulse Output: 1 m³ / Pulse	OFF	ON	OFF							
Function Reserved	OFF	OFF	ON							

7.0 Parameter set

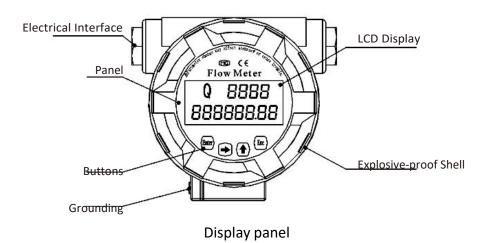



7.1There are four keys: "Enter", " \rightarrow ", " \uparrow ", "Esc".

KEYS	Description			
Enter	Save the value and advance to next menu			
\rightarrow	For numerical values, move cursor position			
1	To change number unit, setting			
Esc	Return to measuring model			

7.2 Description of Password Grade

Password	Description			
1234	Modify parameters			
5555	Total rate reset			

7.3 Description of menu

Menu	Parameter	Setting Method	Grade	Description		
F-1	Unit	Select parameter	User	Value	Flow Unit	Total Flow Unit
				0	M3/h	M3
				1	L/h	L
				2	L/min	L
				3	US Gal/min	US Gal
				4	UK Gal/min	UK Gal
				5	US Gal/h	US Gal
				6	UK Gal/min	UK Gal



B t/h T 9 Ft3/h Ft3					7	KG/h	Kg
Province							
F-2 Damp time Input value User Unit: Second Value: 0-996 F-3 Max flow rate Input value User Unit: The same to the F-1 F-4 Min flow rate Input value User When the flow rate lower than min flow rate, the flow rate will display 0; The unit is the same to the F-1 F-5 Max frequency output Input value User Accuracy: 0.1Hz When need to display mass unit, it needs to input the density of liquid. The unit of density is g/cm3 F-7 Pulse output Select parameter User User User User User Parameter User User User User User User User Us						,	·
F-2 Damp time Input value User Value: 0°-99s					_	FLS/II	FLS
F-3 Max flow rate Input value User When the flow rate lower than min flow rate, the flow rate will display 0; The unit is the same to the F-1 When the flow rate lower than min flow rate, the flow rate will display 0; The unit is the same to the F-1 When need to display mass unit, it needs to input the density of liquid. The unit of density is g/cm3 Pulse output Select parameter User Select parameter User parameter F-8 Scaled pulse Select parameter User parameter F-9 Pulse width Input value Select parameter F-10 Communication Select parameter User Select parameter F-11 Baud Select parameter User Select parameter Select parameter User Select parameter Sel	F-2	Damp time	Input value	User			
F-5 Max frequency output Input value User Accuracy: 0.1Hz F-6 Density Input value User Accuracy: 0.1Hz F-7 Pulse output Select parameter User Scaled pulse User User User User User User User Us	F-3	Max flow rate	Input value	User		e to the F-1	
F-5 Max frequency output Input value User Accuracy: 0.1Hz F-6 Density Input value User Accuracy: 0.1Hz F-7 Pulse output Select parameter User Scaled pulse User User User User User User User Us	Γ 4	NA:n flavorate	la a de calco	Llaan	When the flow	rate lower than min	flow rate, the flow
F-6 Density Input value Select Parameter	F-4	IVIIN flow rate	input value	User			
F-7 Pulse output Select parameter F-8 Scaled pulse Select parameter F-9 Pulse width Input value Select parameter F-10 Communication Select parameter F-11 Baud Select parameter F-12 Total flow Input value P1 Linearization of the Flowcurve: point 1 P2 Linearization of the Flowcurve: point 2 P3 Linearization of the Flowcurve: point 3 Flowcurve: point 4 P5 Linearization of the Flowcurve: point 4 P6 Linearization of the Flowcurve: point 5 F-16 Linearization of the Flowcurve: point 5 F-17 Linearization of the Flowcurve: point 5 F-18 Linearization of the Flowcurve: point 5 F-19 Linearization of the Flowcurve: point 5 F-10 Linearization of the Flowcurve: point 6 Linearization of the Flowcurve: point 7 Flowcurve: point 7 Flowcurve: point 8 Linearization of the Flowcurve: point 6 Flowcurve: point 7 Flowcurve: point 8 Linearization of the Flowcurve: point 7 Flowcurve: point 8 Linearization of the Flowcurve: point 6 Flowcurve: point 7 Flowcurve: point 8 Linearization of the Flowcurve: point 7 Flowcurve: point 8 Linearization of the Flowcurve: point 6 Flowcurve: point 7 Flowcurve: point 8 Linearization of the Flowcurve: point 9 Flowcurve: point 10 Flowcurve: point 10 Flowcurve: point 10 Flowcurve: point 10 Flowcurve: p	F-5	Max frequency output	Input value	User			
F-7 Pulse output Select parameter Select parameter F-8 Scaled pulse Select parameter F-9 Pulse width Input value Select parameter F-10 Communication Select parameter Select parameter F-11 Baud F-12 Total flow Input value P1 Linearization of the Flowcurve: point 1 P2 Linearization of the Flowcurve: point 2 P3 Linearization of the Flowcurve: point 3 F-14 Linearization of the Flowcurve: point 4 F-15 Linearization of the Flowcurve: point 5 F-16 Linearization of the Flowcurve: point 5 F-17 Linearization of the Flowcurve: point 6 F-18 Linearization of the Flowcurve: point 5 F-19 Linearization of the Flowcurve: point 6 F-10 Linearization of the Flowcurve: point 1 F-10 Linearization of the Flowcurve: point 3 F-10 Linearization of the Flowcurve: point 4 F-10 Linearization of the Flowcurve: point 5 F-10 Linearization of the Flowcurve: point 6 Linearization of the Flowcurve: point 7 F-10 Linearization of the Flowcurve: point 6 Linearization of the Flowcurve: point 7 F-10 Linearization of the Flowcurve: point 6 Linearization of the Flowcurve: point 7 F-10 Linearization of the Flowcurve: point 6 Linearization of the Flowcurve: point 7 F-10 Linearization of the Flowcurve: point 6 Linearization of the Flowcurve: point 7 F-10 Linearization of the Flowcurve: point 8 Linearization of the Flowcurve: point 6 Linearization of the Flowcurve:	F-6	Density	Innut value	Hear	When need to display mass unit, it needs to input the		
F-8 Scaled pulse Select parameter F-9 Pulse width Input value F-10 Communication Select parameter Select parameter F-11 Baud F-12 Total flow Input value P1 Linearization of the Flowcurve: point 1 P2 Linearization of the Flowcurve: point 2 P3 Linearization of the Flowcurve: point 3 F-14 Linearization of the Flowcurve: point 3 F-15 Linearization of the Flowcurve: point 4 F-16 Linearization of the Flowcurve: point 5 F-17 Linearization of the Flowcurve: point 5 F-18 Linearization of the Flowcurve: point 5 F-19 Linearization of the Flowcurve: point 6 F-10 Linearization of the Flowcurve: point 9 Elinearization of the Flowcurve: point 1 F-17 Linearization of the Flowcurve: point 3 F-18 Linearization of the Flowcurve: point 4 F-19 Linearization of the Flowcurve: point 5 F-10 Linearization of the Flowcurve: point 6 F-10 Linearization of the Flowcurve: point 6 Linearization of the Flowcurve: point 7 F-10 Linearization of the Flowcurve: point 6 Linearization of the Flowcurve: point 7 F-10 Linearization of the Flowcurve: point 7 F-10 Linearization of the Flowcurve: point 6 Linearization of the Flowcurve: point 7 F-10 Linearization of the Flowcurve: point 7 F-10 Linearization of the Flowcurve: point 7 F-10 Linearization of the Flowcurve: point 6 Linearization of the Flowcurve: point 7 F-10 Linearization of the Flowcurve: point 7 F-10 Linearization of the Flowcurve: point 7 F-10 Linearization of the Flowcurve: point 6 L	1-0	Delisity	•	0361			
F-8 Scaled pulse Scaled pulse Select parameter Select parameter F-9 Pulse width F-10 Communication Select parameter Select paramete	F-7	Pulse output	Select	User		•	
F-8 Scaled pulse Select parameter User Pulse width Input value F-9 Pulse width Input value F-10 Communication Select parameter F-11 Baud F-11 Baud F-12 Total flow Input value P1 Linearization of the Flowcurve: point 1 F-12 Linearization of the Flowcurve: point 3 F-13 Flowcurve: point 3 P4 Linearization of the Flowcurve: point 5 F-14 Linearization of the Flowcurve: point 5 F-15 Linearization of the Flowcurve: point 5 P5 Linearization of the Flowcurve: point 5 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 6 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 6 P8 Linearization of the Flowcurve: point 6 P9 Linearization of the Flowcurve: point 6 P1 Linearization of the Flowcurve: point 9 P2 Linearization of the Flowcurve: point 1 P3 Linearization of the Flowcurve: point 4 P5 Linearization of the Flowcurve: point 5 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 6 P8 Linearization of the Flowcurve: point 6 P9 Linearization of the Flowcurve: point 6 P9 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P9 Coefficient P1 Linearization of the Flowcurve: point 6 P9 Linearization of the Flowcurve: point 6 P0 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P9 Linearization of the Flowcurve: point 8 P8 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P9 Linearization of the Flowcurve: point 8 P1 Linearization of the Flowcurve: point 8 P8 Linearization of the Flowcurve: point 8 P9 Linearization of the Flowcurve: point 8 P9 Linearization of the Flowcurve: point 8 P0 Linearization of the Flowcurve: point 9 P0 Linearization of the Flowcurve: point 9 P1 Linearization 0 The Flowcurve: point 9 P1 Linearization 0 The Flowcurve: point 9 P1 Linear			parameter				
F-8 Scaled pulse						·	
F-9 Pulse width Input value F-10 Communication Select parameter F-11 Baud F-12 Total flow Input value P1 Linearization of the Flowcurve: point 2 P3 Linearization of the Flowcurve: point 3 P4 Linearization of the Flowcurve: point 4 P5 Linearization of the Flowcurve: point 5 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P9 Coefficient P9 Coefficient P9 Coefficient P9 Coefficient P1 Linearization of the Flowcurve: point 3 P9 Linearization of the Flowcurve: point 4 P5 Linearization of the Flowcurve: point 5 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P9 Coefficient P1 Linearization of the Flowcurve: point 8 P9 Coefficient P1 Linearization of the Flowcurve: point 6 P1 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P9 Coefficient P1 Linearization P1 Linearization P1 Linearization P1 Linearization P1 Linearization P2 Linearization P3 Linearization P4 Linearization P5 Linearization P6 Linearization P7 Linearization P7 Linearization P8 Linearization P8 Linearization P9 Linearization P1 Linearization P1 Linearization P1 Linearization P1 Li			Select				
F-9 Pulse width Input value User 1: 1 unit volume / pulse F-10 Communication Select parameter User Select parameter Select parameter User Select parameter Select parameter User Select parameter Select parameter Select parameter User Select parameter Select parameter Select parameter User Select parameter S	F-8	Scaled pulse		User			
F-9 Pulse width Input value User Select parameter User Select Select parameter User Select parameter User Select parameter User Select Select parameter User Select Select parameter User Select Select parameter User Select Select Select parameter User Select Select Select parameter User Select Sele			parameter				
F-10 Communication Select parameter F-11 Baud Select parameter F-12 Total flow Input value P1 Linearization of the Flowcurve: point 3 F-15 Linearization of the Flowcurve: point 4 P2 Linearization of the Flowcurve: point 3 F-16 Linearization of the Flowcurve: point 4 P1 Linearization of the Flowcurve: point 5 F-17 Linearization of the Flowcurve: point 6 P2 Linearization of the Flowcurve: point 7 P3 Linearization of the Flowcurve: point 8 P4 Linearization of the Flowcurve: point 5 Linearization of the Flowcurve: point 6 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P9 Linearization of the Flowcurve: point 8 P1 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 8 P8 Linearization of the Flowcurve: point 8 P9 Coefficient P					• •		
F-10 Communication Select parameter F-11 Baud Select parameter F-12 Total flow Input value P1 Linearization of the Flowcurve: point 1 P2 Linearization of the Flowcurve: point 2 P3 Linearization of the Flowcurve: point 3 P4 Linearization of the Flowcurve: point 4 P5 Linearization of the Flowcurve: point 5 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 6 P8 Linearization of the Flowcurve: point 6 P9 Linearization of the Flowcurve: point 8 P9 Linearization of the Flowcurve: point 6 P1 Linearization of the Flowcurve: point 8 P3 Linearization of the Flowcurve: point 9 Linearization of the Flowcurve: point 9 Linearization of the Flowcurve: point 5 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P9 Coefficient Linearization of the Flowcurve: point 8 P9 Linearization of the Flowcurve: point 8 P8 Linearization of the Flowcurve: point 8 P9 Coefficient Linearization of the Flowcurve: point 8 P8 Linearization of the Flowcurve: point 8 P9 Coefficient Linearization of the Flowcurve: point 8 P8 Linearization of the Flowcurve: point 8 P9 Coefficient Linearization of the Flowcurve: point 8 P9 Coefficient Linearization of the Flowcurve: point 8 Lineariz	F-9	a Pulse width Input value User				nge, and it's multiple	
F-10 Communication Parameter User Baud rate: 1200, 2400, 4800, 9600, 19200		1 2 2 2 2 2 2 2 2 2 2 2 2 2 2 2 2 2 2 2					
F-11 Baud Select parameter User P1 Linearization of the Flowcurve: point 2 P3 Linearization of the Flowcurve: point 3 P4 Linearization of the Flowcurve: point 4 P1 Linearization of the Flowcurve: point 5 P5 Linearization of the Flowcurve: point 5 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 6 P8 Linearization of the Flowcurve: point 6 P9 Linearization of the Flowcurve: point 6 P1 Linearization of the Flowcurve: point 5 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 6 P8 Linearization of the Flowcurve: point 6 P9 Linearization of the Flowcurve: point 6 P1 Linearization of the Flowcurve: point 7 P1 Linearization of the Flowcurve: point 8 P1 Linearization of the Flowcurve: point 8 P2 Linearization of the Flowcurve: point 6 P3 Linearization of the Flowcurve: point 6 P4 Linearization of the Flowcurve: point 6 P5 Linearization of the Flowcurve: point 6 P6 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P9 Linearization of the Flowcurve: point 8 P1 Linearization of the Flowcurve:	F-10	Communication		User			
F-11 Baud Select parameter User E (Even verify)			parameter			0, 2400, 4800, 9600,	19200
F-11 Baud Select parameter User E(Even verify) Data length: 7,8 Stop bits length: 1,2				User	'		
P-1 Linearization of the Flowcurve: point 3 Linearization of the Flowcurve: point 4 Linearization of the Flowcurve: point 5 Linearization of the Flowcurve: point 6 Linearization of the Flowcurve: point 6 Linearization of the Flowcurve: point 6 Linearization of the Flowcurve: point 7 Linearization of the Flowcurve: point 8 Linearization of the Flowcurve: point 7 Linearization of the Flowcurve: point 7 Linearization of the Flowcurve: point 7 Linearization of the Flowcurve: point 8 Li		Baud			· · · · · · · · · · · · · · · · · · ·		
F-12 Total flow Input value User It could be modified with right code P1 Linearization of the Flowcurve: point 1 P2 Linearization of the Flowcurve: point 2 P3 Linearization of the Flowcurve: point 3 P4 Linearization of the Flowcurve: point 4 P5 Linearization of the Flowcurve: point 5 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P9 Coefficient P7 Linearization of the Flowcurve: point 8 P9 Coefficient P7 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P9 Coefficient P7 Linearization of the Flowcurve: point 8 P9 Coefficient P7 Linearization of the Flowcurve: point 8 P9 Coefficient P7 Linearization Of the Flowcu	F-11				i i i i i i i i i i i i i i i i i i i		
F-12 Total flow Input value User It could be modified with right code P1 Linearization of the Flowcurve: point 1 P2 Linearization of the Flowcurve: point 2 P3 Linearization of the Flowcurve: point 3 P4 Linearization of the Flowcurve: point 4 P5 Linearization of the Flowcurve: point 5 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P9 Coefficient P1 Linearization of the Flowcurve: point 8 P9 Coefficient P0 Coefficient P1 Linearization of the Flowcurve: point 6 P1 Linearization of the Flowcurve: point 6 P2 Linearization of the Flowcurve: point 6 P3 Linearization of the Flowcurve: point 5 P4 Linearization of the Flowcurve: point 5 P5 Linearization of the Flowcurve: point 6 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P9 Coefficient							
P1							
Flowcurve: point 1 P2 Linearization of the Flowcurve: point 2 P3 Linearization of the Flowcurve: point 3 P4 Linearization of the Flowcurve: point 4 P5 Linearization of the Flowcurve: point 5 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P6 Coefficient P7 Coefficient P8 Coefficient P8 Coefficient P9 Coefficient P8 Coefficient P9 Coefficient P9 Coefficient P9 Coefficient P8 Linearization of the Flowcurve: point 8 P9 Coefficient P9 Coefficient P8 Linearization of the Flowcurve: point 8 P9 Coefficient P9 Coefficient P9 Coefficient P9 Coefficient P9 Coefficient P8 Linearization of the Flowcurve: point 8 P9 Coefficient P9 Coe	F-12		Input value		_		
Flowcurve: point 1 P2 Linearization of the Flowcurve: point 2 P3 Linearization of the Flowcurve: point 3 P4 Linearization of the Flowcurve: point 4 P5 Linearization of the Flowcurve: point 5 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P6 Coefficient P7 Coefficient P8 Coefficient P8 Coefficient P9 Coefficient P9 Coefficient P8 Linearization of the Flowcurve: point 8 P9 Coefficient P9 Coefficient P8 Linearization of the Flowcurve: point 8 P9 Coefficient P9 Coefficient P8 Linearization of the Flowcurve: point 8 P9 Coefficient P9 Coefficient P8 Linearization of the Flowcurve: point 8 P9 Coefficient P9 Coefficient P9 Coefficient P8 Linearization of the Flowcurve: point 8 P9 Coefficient P9 Coefficient P9 Coefficient P9 Coefficient P8 Linearization of the Flowcurve: point 8 P9 Coefficient P9 Coefficient P9 Coefficient P9 Coefficient P9 Coefficient P9 Coefficient P8 Linearization of the Flowcurve: point 8 P9 Coefficient P9 Coe	P1	l .	Input value		• • • • • • • • • • • • • • • • • • • •		•
Flowcurve: point 2 P3 Linearization of the Flowcurve: point 3 P4 Linearization of the Flowcurve: point 4 P5 Linearization of the Flowcurve: point 5 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P8 Coefficient P9 Coefficient Flowcurve: point 8 Flowcurve: point 9 Flowcurve: point 6 Flowcurve:		•	1				
Flowcurve: point 2 P3 Linearization of the Flowcurve: point 3 P4 Linearization of the Flowcurve: point 4 P5 Linearization of the Flowcurve: point 5 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P8 Coefficient P9 Coefficient Flowcurve: point 8 Factory First Row: Corrected Frequency (F4) without decimal, Second Row: Coefficient error with (K4) six decimals Factory First Row: Corrected Frequency (F5) without decimal, Second Row: Coefficient error with (K5) six decimals Factory First Row: Corrected Frequency (F6) without decimal, Second Row: Coefficient error with (K6) six decimals Factory First Row: Corrected Frequency (F6) without decimal, Second Row: Coefficient error with (K6) six decimals Factory First Row: Corrected Frequency (F7) without decimal, Second Row: Coefficient error with (K7) six decimals Factory First Row: Corrected Frequency (F8) without decimal, Second Row: Coefficient error with (K8) six decimals Factory First Row: Corrected Frequency (F8) without decimal, Second Row: Coefficient error with (K8) six decimals Factory First Row: Corrected Frequency (F8) without decimal, Second Row: Coefficient error with (K8) six decimals Factory First Row: Corrected Frequency (F8) without decimal, Second Row: Coefficient error with (K8) six decimals First Row: Corrected Frequency (F8) without decimal, Second Row: Coefficient error with (K8) six decimals First Row: Corrected Frequency (F8) without decimal, Second Row: Coefficient error with two decimals, Second Row: Coefficient error with two decimals	P2	I IIIDUI VAIDE					
Flowcurve: point 3 P4 Linearization of the Flowcurve: point 4 P5 Linearization of the Flowcurve: point 5 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P9 Coefficient Flowcurve: point 8 Flowcurve: point 9 Flowcurve: point 6 Flowcurve: point 7 Flowcurve: point 6 Flowcurve: point 7 Flowcurve: point 6 Flowcurve: point 7 Flowcurve: point 6 Flowcurve:			•				
Linearization of the Flowcurve: point 4 Input value Factory only Second Row: Coefficient error with (K4) six decimals	Р3		Input value	1	.		
Flowcurve: point 4 P5 Linearization of the Flowcurve: point 5 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P9 Coefficient Flowcurve: point 8 Factory First Row: Corrected Frequency (F5) without decimal, Second Row: Coefficient error with (K5) six decimals Factory First Row: Corrected Frequency (F6) without decimal, Second Row: Coefficient error with (K6) six decimals Factory First Row: Corrected Frequency (F7) without decimal, Second Row: Coefficient error with (K7) six decimals Factory First Row: Corrected Frequency (F8) without decimal, Second Row: Coefficient error with (K8) six decimals Factory First Row: Corrected Frequency (F8) without decimal, Second Row: Coefficient error with (K8) six decimals Factory First Row: Corrected Frequency (F8) without decimal, Second Row: Coefficient error with (K8) six decimals Factory Only First Row: Corrected Frequency with one decimal, Second Row: Coefficient error with two decimals, unit:							
Linearization of the Flowcurve: point 5 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P7 Coefficient P8 Coefficient P8 Coefficient P9 Coefficient P8 Linearization of the Flowcurve: point 8 P8 Coefficient P8 Linearization of the Flowcurve: point 8 P9 Coefficient P8 Linearization of the Flowcurve: point 8 P8 Linearization of the Flowcurve: point 8 P9 Coefficient P8 Linearization of the Flowcurve: point 8 P9 Coefficient P8 Linearization of the Flowcurve: point 8 P9 Coefficient P8 Linearization of the Flowcurve: point 8 P9 Coefficient P8 Linearization of the Flowcurve: point 8 P9 Coefficient P8 Linearization of the Flowcurve: point 8 P9 Coefficient P9 Coefficient P8 Linearization of the Flowcurve: point 8 P9 Coefficient P9 Coeffi	P4		Input value	1			
Flowcurve: point 5 P6 Linearization of the Flowcurve: point 6 P7 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P9 Coefficient Flowcurve: point 8 Factory First Row: Corrected Frequency (F6) without decimal, Second Row: Coefficient error with (K6) six decimals Factory First Row: Corrected Frequency (F7) without decimal, Second Row: Coefficient error with (K7) six decimals Factory First Row: Corrected Frequency (F8) without decimal, Second Row: Coefficient error with (K8) six decimals Factory First Row: Corrected Frequency (F8) without decimal, Second Row: Coefficient error with (K8) six decimals Factory First Row: Corrected Frequency (F8) without decimal, Second Row: Coefficient error with (K8) six decimals First Row: Corrected Frequency with one decimal, Second Row: Coefficient error with two decimals, unit:			Input value	Factory			
Linearization of the Flowcurve: point 6 Input value Factory only Second Row: Corrected Frequency (F6) without decimal, Second Row: Coefficient error with (K6) six decimals	P5				, , , ,		
Flowcurve: point 6 P7 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P9 Coefficient P7 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P9 Coefficient P7 Linearization of the Flowcurve: point 8 P8 Linearization of the Flowcurve: point 8 P9 Coefficient P8 Linearization of the Flowcurve: point 8 P9 Coefficient P9 Coefficient P8 Linearization of the Flowcurve: point 8 P6 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P6 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 P6 Linearization of the Flowcurve: point 8 P7 Linearization of the Flowcurve: point 8 P6 Linearization of the Flowcurve: point 8 P6 Linearization of the Flowcurve: point 8 P7 Linearization of the Flowcurve: point 8 P6 Linearization of the Flowcurve: point 8 P7 Linearization of the Flowcurve: point 8 P6 Linearization of the Flowcurve: point 8 P7 Linearization			Input value				
P7 Linearization of the Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 Linearization of the Flowcurve: point 7 Linearization of the Flowcurve: point 8 Linearization of the Flowcurve:	P6			1			
Flowcurve: point 7 P8 Linearization of the Flowcurve: point 8 Input value P9 Coefficient Input value Input value Input value Factory only First Row: Corrected Frequency with one decimal, Second Row: Coefficient error with two decimals, unit:							
P8 Linearization of the Flowcurve: point 8 Input value Pactory Only Second Row: Corrected Frequency (F8) without decimal, Second Row: Coefficient error with (K8) six decimals Factory Only First Row: Corrected Frequency with one decimal, Second Row: Coefficient error with two decimals, unit:	Р7	l .	Input value	1			
Flowcurve: point 8 only Second Row: Coefficient error with (K8) six decimals Factory only Second Row: Coefficient error with (K8) six decimals Factory only Second Row: Coefficient error with two decimals, unit:		·		<u> </u>			
P9 Coefficient Input value Factory only First Row: Corrected Frequency with one decimal, Second Row: Coefficient error with two decimals, unit :	P8	I .	Input value	1			
P9 Coefficient Input value only Second Row: Coefficient error with two decimals, unit:		1.000carve. point o		Only	1		` ,
Only Only	DC	Coefficient	Input value	1			
	P9	Coefficient				oefficient error with	two decimals, unit :
				,	/L, K		




8.0 TROUBLESHOOTING

Symptom	Probable Cause	Solution		
Measurement is	1. Turbine operated below minimum	Increase flow rate. Refer to Section 3.0		
not accurate	rate.	Operation Conditions		
	, , ,	Remove turbine. Clean carefully. Make rotor spins freely.		
	3. Installed too close to fittings.	Install correctly. Refer to Section 5.0 Cautions for Installation		
LCD Display	1. Battery Power Type: Bad contact on	Open back cover and repower the flow		
Abnormality	the connector between battery and PCB	meter		
	2. DC Power Type: supply voltage is abnormal	Check and en power supply is 24V DC		



METER CONSTRUCTION 9.0

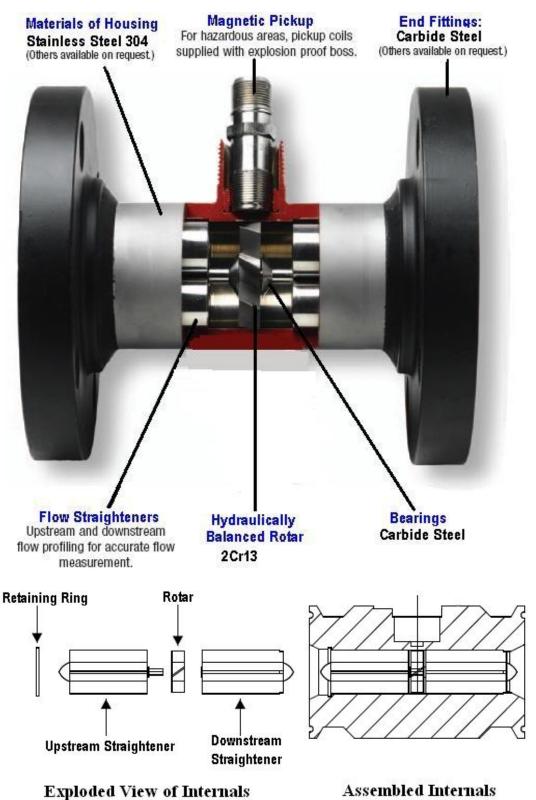



Limited Warranty Policy

Hereby provides a limited warranty against defects in materials and workmanship. This product includes a one-year warranty. The warranty period shall begin on the date of the original new equipment purchase. Warrantor's obligation hereunder shall be limited to repairing defective workmanship or replacing or repairing any defective parts.

In the event Purchaser believes the product is defective, the product must be returned to, transportation prepaid by Purchaser, within the appropriate warranty period relative to the product. If 's inspection determines the workmanship or materials are defective and the required maintenance has been performed and, has been properly installed and operated, the product will be either repaired or replaced, at 's sole determination, free of additional charge, and the goods will be returned, transportation paid by , using a transportation method selected by .

Prior to returning the product to , Purchaser must obtain a Returned Material Authorization (RMA) Number from 's Customer Service Department within 30 days after discovery of a purported breach of warranty, but not later than the warranty period; otherwise, such claims shall be deemed waived.

If 's inspection reveals the product to be free of defects in material and workmanship or such inspection reveals the goods were improperly used, improperly installed,and/or improperly selected for service intended,will notify the purchaser in writing and will deliver the goods back to Purchaser upon receipt of Purchaser's written instructions and agreement to pay the cost of transportation. If Purchaser does not respond within thirty (30) days after notice from , the goods will be disposed of in 's discretion.

does not warrant the product to meet the requirements of any safety code or other jurisdiction, and Purchaser assumes all risk and liability whatsoever resulting from the use thereof, whether used singly or in combination with other machines or apparatus.

This warranty shall not apply to any product or parts thereof, which have been repaired outside 's factory or altered in any way, or have been subject to misuse, negligence, or accident, or have not been operated in accordance with 's printed instructions or have been operated under conditions more severe than, or otherwise exceeding, those set in the specifications.

FOR NON- WARRANTY REPAIRS OR CALIBRATIONS, consult for current repair/calibration charges. Have the following information available BEFORE contacting:

- 1.P.O. number to cover the COST of the repair/calibration,
- 2. Model and serial number of the product, and
- 3. Repair instructions and/or specific problems relative to the product.